



CERTIFICATE OF ACCREDITATION

The ANSI National Accreditation Board

Hereby attests that

Accurate Calibration, Inc.
9735 Alpaca Street
South El Monte, CA 91733

Fulfills the requirements of

ISO/IEC 17025:2017

and national standard

ANSI/NCSL Z540-1-1994 (R2002)

In the field of

CALIBRATION

This certificate is valid only when accompanied by a current scope of accreditation document.
The current scope of accreditation can be verified at www.anab.org.

Jason Stine, Vice President

Expiry Date: 07 December 2026
Certificate Number: AC-1240



This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2017.
This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory
quality management system (refer to joint ISO-ILAC-IAF Communiqué dated April 2017).

SCOPE OF ACCREDITATION TO ISO/IEC 17025:2017

AND

ANSI/NCSL Z540-1-1994 (R2002)

Accurate Calibration, Inc.

9735 Alpaca Street
South El Monte, CA 91733
Guy Uriel (626) 762-1520

CALIBRATION

Valid to: **December 7, 2026**

Certificate Number: **AC-1240**

Chemical Quantities

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
pH Meters ¹	2 to 12 pH	0.026 pH	Comparison to Accredited pH Buffer Solutions
Viscosity Cups ¹	30 to 530 cSt	2.6 % of reading	Comparison to Viscosity Standards, Stopwatch

Electrical – DC/Low Frequency

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Temperature – Digital Indicator	Type J (32 to 1 112) °F	0.22 °F	Fluke 8842A 5.5 Digit Multimeter; AMS 2750H
	Type K (32 to 2 400) °F	0.28 °F	
	Type N (32 to 2 400) °F	0.41 °F	
	Type R (32 to 2 400) °F	2 °F	
	Type S (32 to 2 400) °F	2 °F	
	Type T (-300 to 392) °F	0.3 °F	

Electrical – DC/Low Frequency

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Thermocouple Temperature Simulation ¹ (Controllers and Recorders)	Type J (-200 to 2 100) °F	0.72 °F	Fluke 724 Process Calibrator; AMS 2750H
	Type K (-200 to 2 400) °F	0.74 °F	
	Type N (-200 to 2 100) °F	0.73 °F	
	Type R (-4 to 3 100) °F	1.4 °F	
	Type S (-4 to 3 100) °F	1.4 °F	
	Type T (-328 to 750) °F	0.73 °F	

Mass and Mass Related

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Pressure Gauges (Hydraulic)	(0 to 10 000) psi (10 000 to 15 000) psi	3.6 psi 3.8 psi	Comparison to Additel 680 Digital Pressure Gauge
Vacuum Sensors/Gauges (Pneumatic)	(0.0001 to 0.1) Torr	5.8 % of reading	Comparison to MKS Baratron Capacitance Manometer
Vacuum Sensors/Gauges (Pneumatic)	(0.1 to 1) Torr	5.3 % of reading + 3.4 mTorr	Comparison to MKS Baratron Capacitance Manometer
Vacuum Sensors/Gauges (Pneumatic)	(1 to 750) Torr	5.1 % of reading + 49 mTorr	Comparison to MKS Baratron Capacitance Manometer
Vacuum Sensors/Gauges (Pneumatic)	(0.01 to 30) inHg	0.047 % of reading + 0.073 inHg	Comparison to Ashcroft 2089 Digital Pressure Gauge
Vacuum Sensors/Gauges ¹ (Pneumatic)	(0.1 to 30) inHg	0.068 % of reading + 0.09 inHg	Comparison to Ashcroft 1082 Test Gauge


Thermodynamic

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Thermocouple Probe Calibration by Comparison	Type J (32 to 1 112) °F Type K (32 to 2 400) °F Type N (32 to 2 400) °F Type R (32 to 2 300) °F Type S (32 to 2 400) °F Type T (-300 to 392) °F	0.81 °F 0.87 °F 0.88 °F 1.44 °F 1.44 °F 0.8 °F	Fluke 725 Process Calibrator, Type S Thermocouple Reference Standard; AMS 2750H
Temperature Uniformity Surveys ¹	(32 to 1 000) °F (1 000 to 1 800) °F (1 800 to 2 400) °F	0.063 % of reading + 3.4 °F 0.28 % of reading + 1.2 °F 0.65 % of reading + 5.5 °F	Yokogawa GP20 Data Recorder, Type K Thermocouples; AMS 2750H
Thermocouples	(32 to 2 400) °F	0.67 °F	Comparison to Type S Thermocouple Reference Standard, Fluke 8842A 5.5 Digit Multimeter, Dry Block Calibrators
Humidity – Measure ¹	(10 to 30) %RH (30 to 50) %RH (50 to 70) %RH (70 to 95) %RH	1 %RH 1.1 %RH 1.3 %RH 1.5 %RH	Comparison to Rotronic HP32/Hygroclip2 Humidity Meter with Probe
Infrared Thermometers (IR)	(-18 to 100) °C	1.5 °C	Comparison to Omega BB701 Blackbody Source (Cavity) $\epsilon = 0.95, \lambda = (8 \text{ to } 14) \mu\text{m}$
Infrared Thermometers (IR)	(100 to 260) °C (260 to 583) °C (583 to 760) °C (760 to 982) °C	2.5 °C 5.2 °C 7.5 °C 10 °C	Comparison to Omega BB-4A Blackbody Source (Cavity) $\epsilon = 0.99, \lambda = (8 \text{ to } 14) \mu\text{m}$

Calibration and Measurement Capability (CMC) is expressed in terms of the measurement parameter, measurement range, expanded uncertainty of measurement and reference standard, method, and/or equipment. The expanded uncertainty of measurement is expressed as the standard uncertainty of the measurement multiplied by a coverage factor of 2 ($k=2$), corresponding to a confidence level of approximately 95%.

Notes:

1. On-site calibration service is available for this parameter, since on-site conditions are typically more variable than those in the laboratory, larger measurement uncertainties are expected on-site than what is reported on the accredited scope.
2. Unless otherwise specified in the far-right column, the calibration procedure utilized in the calibration of the listed parameters have been written internally.
3. This scope is formatted as part of a single document including Certificate of Accreditation No. AC-1240.

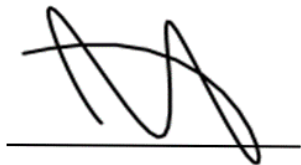

Jason Stine, Vice President

